Lopital Marina
Shower Gurney / Bath Trolley

Battery-Powered Models
Quick Use Instructions

Safety Tips:

- Read the user manual carefully before use (find it at www.lopital.com).
- Maximum load: 396 lbs.
- Make sure the brake is on during patient transfers.
- Check shower bed before each use: mattress intact, no bent or broken parts, and all moving elements function properly.

Use

- Make sure brakes are on.
- Press ‘Up’ for 2 seconds to activate.
- Position stretcher appropriately, using ‘Up’ & ‘Down’ pedals..
- Fold side bar down.*
- Move user to/from the Marina.
- Raise the bed base slightly. Close side bar.*
- Disengage brake to relocate shower bed.
- After 60 minutes inactivity, the Marina will go into sleep mode.

* Use gentle pressure to avoid bending side-release tabs.

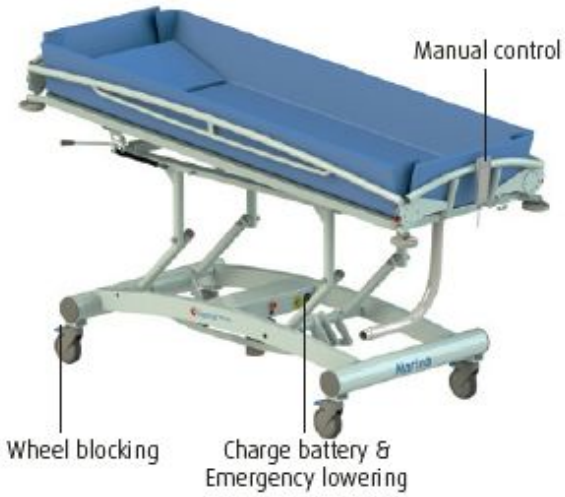

Subject to change without further notice

Battery-Powered Models

Wheel blocking

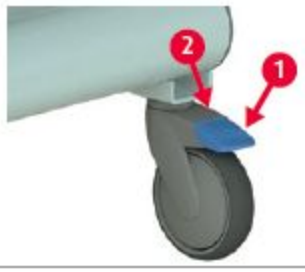

1. Wheel blocking.
2. Unlocking.

Side-bars

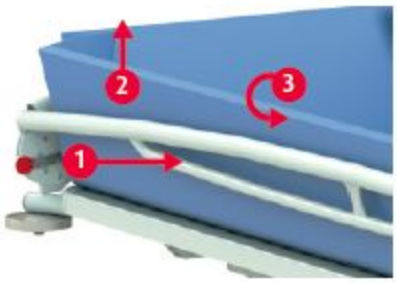

1. Unlock.
2. Tilt.
3. Turn.

When closing, the bar locks automatically.

Emergency lowering (Electric Marina)

If the Marina breaks down, you can lower the stretcher using the emergency lowering button.

Electric manual control

Up

Down

Activate

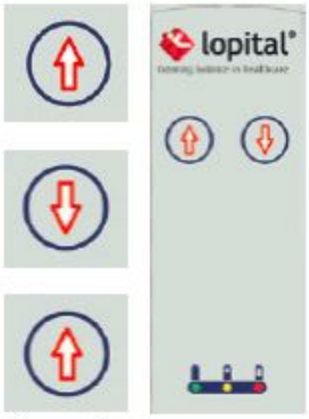

2 seconds

Make sure side bar does not pinch control panel cord.

Charging batteries (Electric Marina)

Connect battery to charger after use.

We recommend charging at the end of each day to keep battery in peak condition.

Cleaning and maintenance

- Clean after every use.
- Use water & regular household cleaners.
- Do not use bleach or abrasive cleaners.
- Check wheels for hairs, debris, & soap residue.

Call us at 800 577-1555 for support or assistance.

Subject to change without further notice

www.max-ability.com 800-577-1555 Fax: 707-575-3856 email: Info@max-ability.com

rev. Nov. 2015